



Quick guide for the Chair Lift



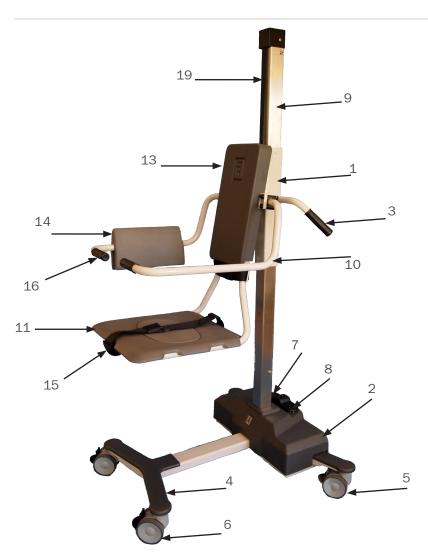



Position	Description
1	Support column
2	Chassis Base
3	Transport handle
4	Chassis leg
5	Positive brake castors, 100mm Twin
6	Straight steering castors, 100mm Twin
7	Foot control for raising
8	Foot control for lowering
9	Stainless Steel column

10	Rotating arm/back supports
11	Hygiene seat and slot
13	"TR" Protection pad
14	Backrest Pad
15	Safety belts
16	Grip
19	Drive belt
20	Low battery audible tone
21	Battery charger input
22	Emergency Stop

Working Load Limit: 150 kg (330 lbs)

Hygiene Equipment Designed for People

TR FOUIPMENT AB TR GROUP INC. TR EQUIPMENT UK LTD.

TR EQUIPMENT

PO Box 116, S-573 22, TRANÅS, SWEDEN 903 WEDEL LANE, GLENVIEW, ILLINOIS 60025, USA INNOVATION CENTRE, GALLOWS HILL, WARWICK CV34 6UW ENGLAND TRANSPOREHAMED GMBH GARTENSTRASSE 9. 42799 LEICHLINGEN. GERMANY

Phone: +1 800-752-6900 Phone: +44 844 335 8386

Fax: +46 140-38 50 61 Phone: +46 140-38 50 60 www.trequipment.com Fax: +1 847-724-8566 Fax: +44 844 335 8383 Phone: +49 2175-16 94 22-0 Fax: +49 2175-16 94 22-19



TR 9650 Mobile Bath Lift System



Quick guide for the Chairlift

- Only qualified staff, who understand all operating and safety procedures may operate the equipment.
- Safety belts must be securely fastened around patient at all times.
- Never leave the patient unattended.
- Castor brakes must be securely locked on the Lifter before transferring a patient on to the chair.
- The patient must be positioned comfortably on the chair, with folded rotating arm.
- Make sure that all parts that come in contact with the patient are intact and without sharp edges.
- Ensure that the Lift can be moved, raised or lowered safely to avoid any pinch injuries to patient.
- Operate the Lift carefully when transporting patients through narrow corridors or over irregular uneven surfaces.
- The TR battery charger is the only one approved for charging.
- Do not use battery charger in wet or damp areas - potential shock hazard.
- It is recommended that the batteries are charged daily or whenever Lifter is not in use. Batteries can not be overcharged.
- Check that castor brakes and straight steering are free from damage.
- Be sure that all details are in place and free from damage and all screws are in place.
- Pads must be kept well maintained in place.
- Lift and chair must be inspected visually for sign of wear. Lift should not be used if defects are noted. Prompt service is required.

Warning: Never use the Lifter in any way that varies from the safety precautions and operating procedures detailed in the operating manual. The equipment must not be operated by anyone until the user has fully read and understands the instructions in the operating manual

Safety autostop mechanism:

If the chair hits an obstacle when lowering, the Lift will safely stop automatically. To release it, just press the "up" right arrow foot control. Same procedure if the lifting belt is slacking. If lifting belt fails, the chair will stop/lock automatically on the column. Call for technical assistance.

For further information see Operating manual

TR EQUIPMENT

TR FOUIPMENT AB TR GROUP INC. TR EQUIPMENT UK LTD.

PO Box 116, S-573 22, TRANAS, SWEDEN 903 WEDEL LANE, GLENVIEW, ILLINOIS 60025, USA INNOVATION CENTRE, GALLOWS HILL, WARWICK CV34 6UW ENGLAND TRANSPOREHAMED GMBH GARTENSTRASSE 9. 42799 LEICHLINGEN. GERMANY

Phone: +46 140-38 50 60 Phone: +1 800-752-6900 Phone: +44 844 335 8386

Fax: +46 140-38 50 61 www.trequipment.com Fax: +1 847-724-8566 Fax: +44 844 335 8383 Phone: +49 2175-16 94 22-0 Fax: +49 2175-16 94 22-19

Hygiene Equipment Designed for People

